

The Journal of Plastination

The official publication of the International Society for Plastination

ISSN 2311-7761



IN THIS ISSUE:


Corrosion Cast of
Bronchopulmonary
Segments – p5

3-D Reconstruction of the
Retrobulbar Orbital Septa
Using Biodur E12®, – p8

Biodur® S10/S3 and
S15/S3 at “Room
Temperature”: a viscosity
study – p15

The Use of Vacuum
Forced Impregnation of
Gum Arabic Solution in
Biological Tissues for
Long-Term Preservation
– p19

Room temperature
Impregnation with Cold
Temperature Biodur®
Silicone: A Study of
Viscosity – p26

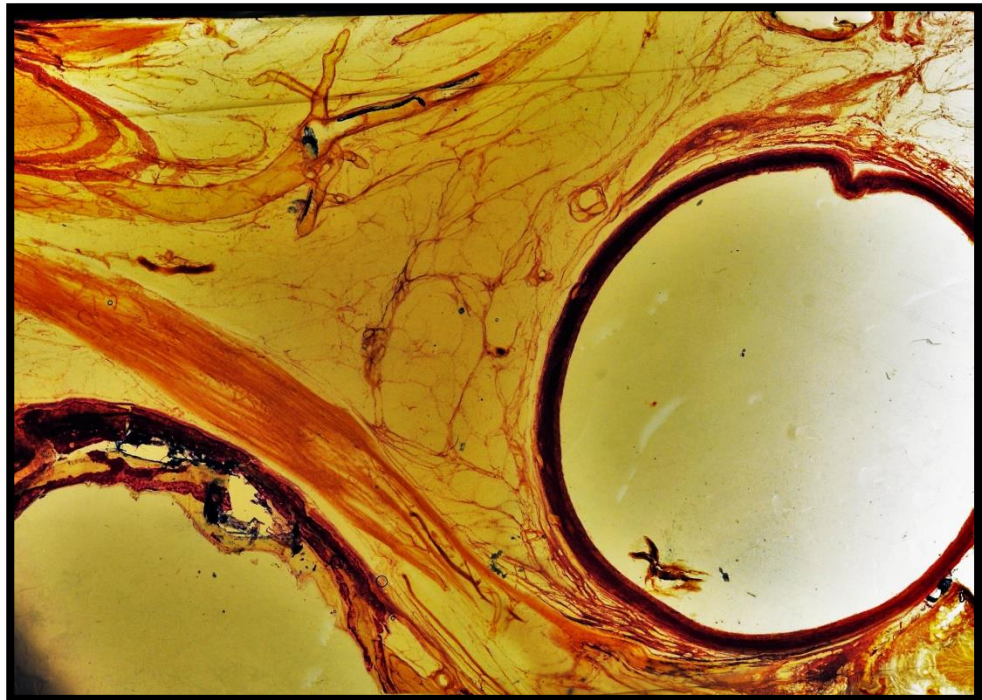

Volume 29 (1); July 2017